



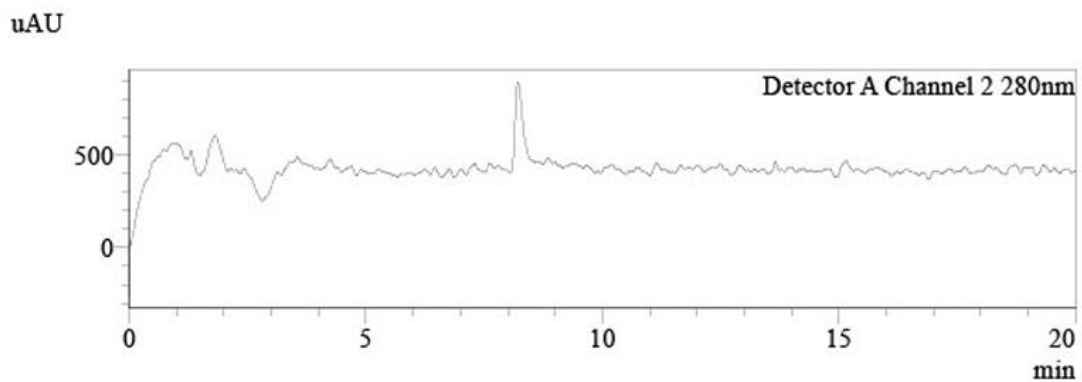

Name: n acetyl semax

Chromatogram

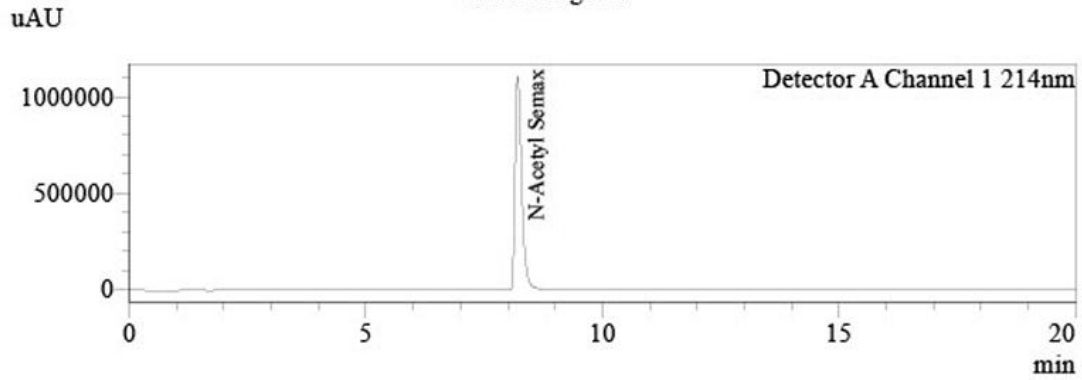

Peak Table

Peak#	Name	Ret. Time	Conc.	Unit	Area%
1		7,386	0,000		0,202
2		7,672	0,000		0,004
3		7,842	0,000		0,020
4	n acetyl semax	8,209	10,761	mg/L	99,775
Total					100,000

Quality Assurance Officer: 李强

Corrector: 佟丽华

Analyst: 刘琼

